

Huntron Workstation Tracker 3200S Tutorial

HUNTRON WORKSTATION TRACKER 3200S TUTORIAL.....	1
Installation Instructions	3
Huntron Workstation Main Interface	4
The Toolbar	5
Hardware Setup	5
Using a Tracker 3200S	6
Manual Modes – Tracker and Scanner	7
Creating a Board Test	8
Converting a Test Created in Workstation 4.2	9
Building Procedures for a New Test	10
Creating a Board Database	10
Adding a New Sequence	11
Adding a New Component	12
Tree/Pin Tab	14
Adding a New Range	15
Scan Results	20
Viewing Signatures – Troubleshoot	21
Viewing Signatures Troubleshoot Report	22
Viewing Signatures – Right Click	24
View SigAssist Information	25
Component Scans Information	26
Component Scans – Right Clicking (Auxiliary menus)	27
Component Scans – Right Clicking (Auxiliary menus)	28
Component Scans – Right Clicking (Auxiliary menus)	29
Sequence/Component/Pin Editing – Right Click menus	30
Pin Editing – Right Clicking (Auxiliary menus)	31
Pin Editing	32
Huntron Workstation Buttons Feature	33
Technical Support	36
Appendix 1: Huntron Workstation Archive Scans Feature	37

Appendix 2: Manually Placing Component Tags in the Image Pane/Image tab39

Huntron Workstation Software Tutorial for Tracker 3200S

It is very helpful if you have a working knowledge of Microsoft Windows prior to using Huntron Workstation.

You are allowed to create a backup copy of the software disk. *Your purchase agreement allows for copies to be made for backup purposes only- copying for distribution or resale is strictly prohibited.*

Installation Instructions

Refer to the Getting Started document included with the Tracker 3200S for complete instructions on software installation.

Uninstall any previous versions of Workstation prior to installing the new version.

Insert the Huntron Workstation DVD. The DVD should Autorun and begin the installation process. If your PC has Autorun disabled then open a browse window to the CD and select WorkstationSetup.exe. This will begin the installation process.

During the install you will be asked to install additional software for Access Probers. Answer **NO** to these questions if you do not have an Access Prober.

If you purchased CAD Tools then install using the supplied CD. Follow instructions listed in the CAD Tools Tutorial.


If you are using Workstation in conjunction with a digital multimeter, follow the instructions listed in the Workstation DMM Tutorial.

All of the Workstation tutorials are available on the Huntron web site:

www.huntron.com/sales-support/software.htm

Huntron Workstation Main Interface


When starting Huntron Workstation for the first time, you will be prompted for an activation code. Type in the code exactly as it is presented on the installation CD. Huntron Workstation 4 has built-in conversion utilities that enable conversion of board tests created in 3.X versions of Huntron Workstation.

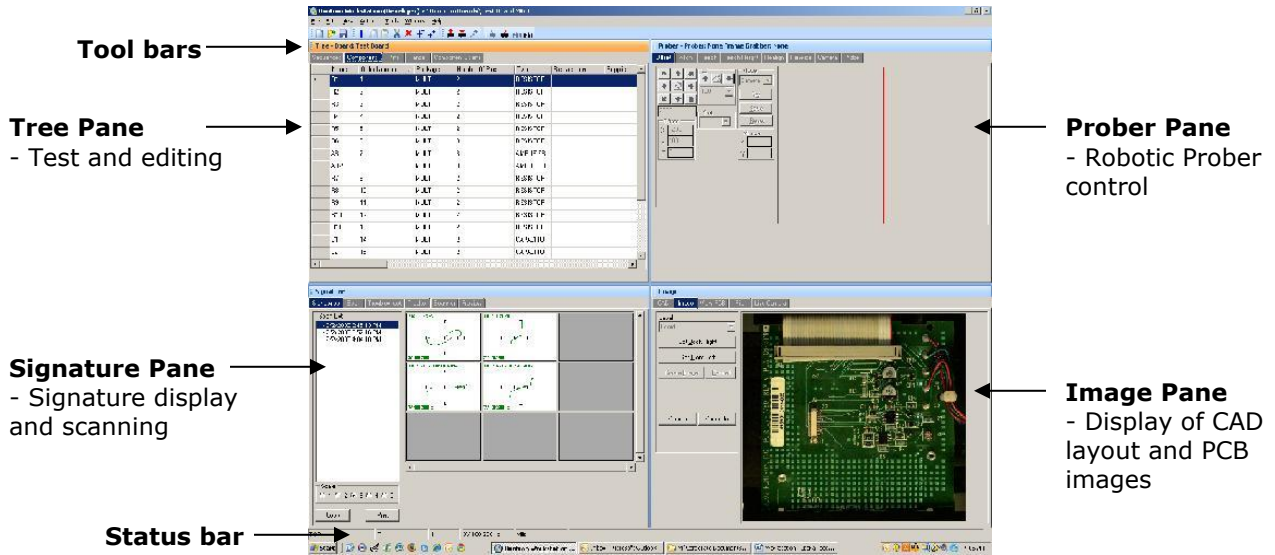

The Main Window for Huntron Workstation 4 features a multi-pane layout so many aspects of the test creation and execution can be displayed at the same time. The Panes are interactive to a certain degree in that changes in one Pane will affect other Panes. The Panes can be resized, floated independently or "tabbed" to the sides of the window. The Status Bar displays information about items currently selected and status information while processes are running.

The Toolbar


The Toolbar just under the application menus allows for quick access to several program functions. The function of each is broken out in the diagram below.

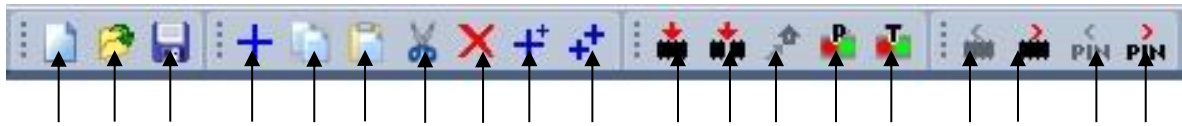

1. 2. 3. 4. 5. 6. 7. 8. 9. 10. 11. 12. 13. 14. 15. 16. 17. 18. 19.


- | | |
|--|---------------------------------------|
| 1. Create New Board database | 11. Scan Component or Net |
| 2. Open Board database | 12. Scan Sequence |
| 3. Save As... | 13. Send Prober head to Home position |
| 4. Add New (Sequence, Component or Range) | 14. Connect/Disconnect Prober |
| 5. Copy (Sequence, Component, Net or Range) | 15. Connect/Disconnect Tracker |
| 6. Paste (Sequence, Component, Net or Range) | 16. Previous Component or Net |
| 7. Cut (Sequence, Component, Net or Range) | 17. Next Component or Net |
| 8. Delete (Seq., Comp., Net, Range or Scan) | 18. Previous Pin |
| 9. Build New (Sequence, Component) | 19. Next Pin |
| 10. Repeat New (Sequence, Component) | |

Hardware Setup

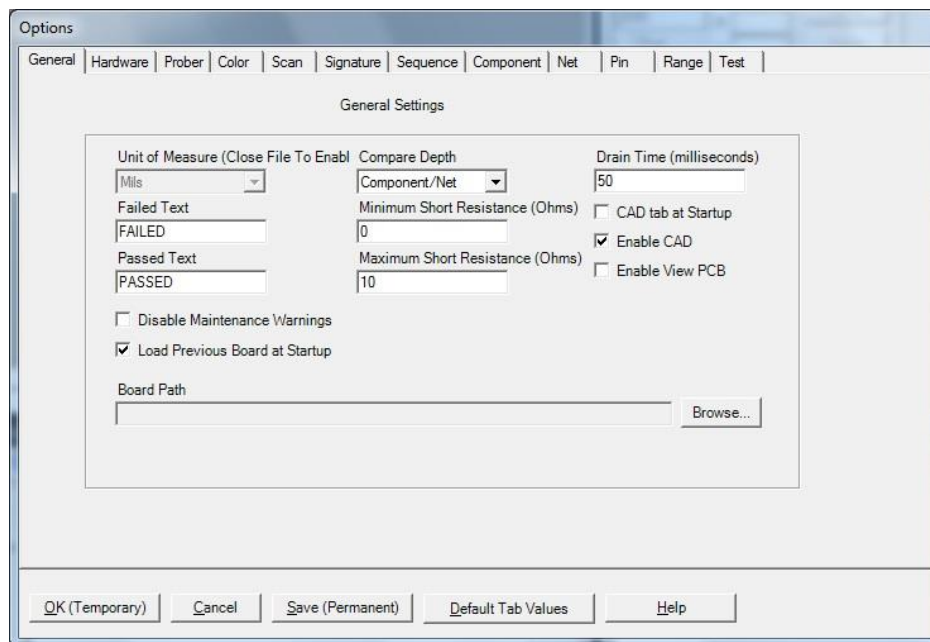

When first starting Huntron Workstation, select **Options** from the **Tools** menu. The Options window is used to setup default settings used when working in Huntron Workstation.

For this tutorial, the Tracker 3200S will be referred to in general as "Tracker".

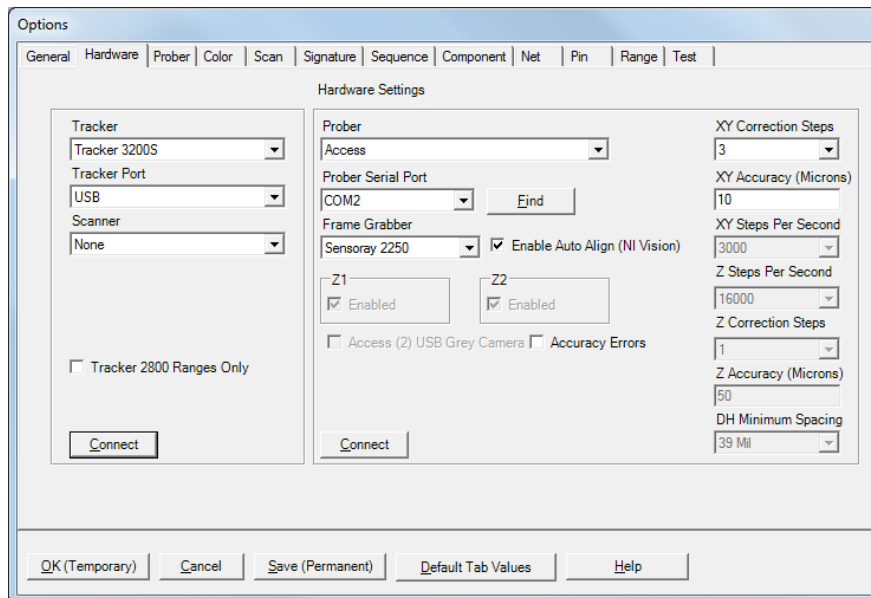

Select **Options** from the **Tools** menu. Select the **Hardware** tab and set the type of Tracker hardware as Tracker 3200S and the Tracker Port as USB. Disregard the Prober settings on the right side of the window.

Click the **Connect** button to initiate communication with the selected hardware. Once connected, the button changes to **Disconnect**. Click the **Save (Permanent)** button to save this configuration as the startup default.

Using a Tracker 3200S


The Tracker 3200S comes from the Factory calibrated for standalone use. If the Tracker 3200S is connected to a Prober or through other cabling connected to the Scanner connections then calibration must be performed.

- Select **Tools/Maintenance/Tracker 3200S Diagnostics** from the menu.

Click the **Alignment** button the Tracker 3200S Diagnostics window. When the Alignment procedure finishes (about 10 minutes), run **Verify Alignment**. This also takes about 10 minutes to complete. The Alignment information is stored in the

Tracker 3200S and will be used by the software. If changes are made to the cabling or attached instruments, simply run **Alignment** and **Verify Alignment** again.

Manual Modes – Tracker and Scanner

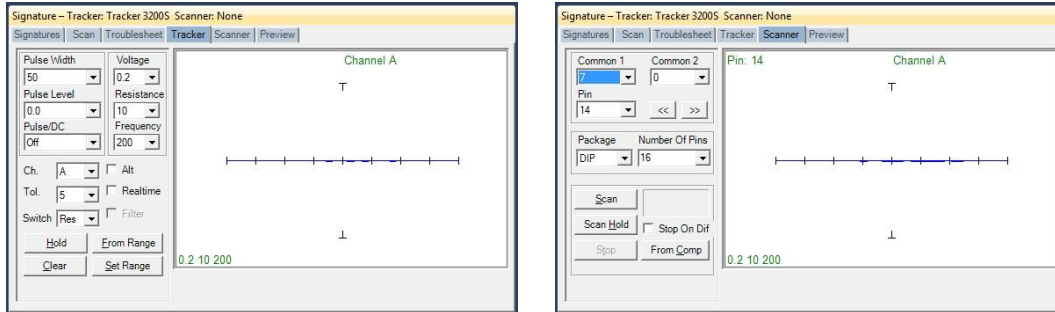

You may find it useful to manually test some of your components while adjusting the range parameters. The two manual modes, Tracker and Scanner located in the **Signatures** pane, can work together to display the signature of a component pin. Tracker mode sets the range parameters, channel, tolerance, footswitch and Pulse Generator settings. Signatures will be displayed to the right while probing with hand-held probes (select the **Realtime** check box). The **Hold** button will capture and hold the current signature allowing for quick comparisons. The **Clear** button will clear the "held" signature.

The **Pulse Width**, **Pulse Level**, **Pulse/DC** settings control the G1 and G2 outputs on the Tracker 3200S front panel. These outputs can be used to bias gated devices such as relays, SCRs and TRIACs.

Scanner mode allows you to use a Tracker 3200S Scanner connections to interface to the component pins. You can set the package type, number of pins and common pins. The **Scan** button starts a hands free scan of the component through the scanner cable interface or you manually increment the pins with the **<<** and **>>** buttons. The **Hold** button will capture and hold the current signature allowing for quick comparisons. Manual modes are for real time display only and does not allow for permanent signature storage. To store signatures you will need to create a **Board Test**.

Creating a Board Test

There are a number of steps necessary to creating a board test.

Workstation Tree Structure

- Board (created Huntron Workstation (.hwdb) database file)
- Sequence (Test set of Components)
- Component or Net (name)
 - o Pins (name, channel)
 - o Ranges (V, F, R range settings)

Example of Board Test Information:

Board Name: Main Board (creates "main board.hwdb" file)

Revision: Rev. A (This field is optional)

Sequence: IC's

Component: U27 (component name) or A2 (NET name)

Pins: per pin settings for Scan Pin setting, channel, net name, etc...

Ranges: Per pin settings for common reference pin, tolerance, etc...


The user has total discretion as to the information input into these fields. There is no "right" way as to what information is entered as every user's situation will be different.

The above example is just one way the information might be entered.


Entering information into the Entry windows is very straight forward. The easiest way to move from field to field is by pressing the **TAB** key. You can also use the mouse to click into a particular field so you can enter information.

Converting a Test Created in Workstation 4.2

Workstation 4.3 uses a different database type than version 4.2. To update a version 4.2 test to work in version 4.3, select **Open** from the **File** menu. In the Open window, select **.MDB** from the file type drop menu. Select the .MDB test file name and click the **Open** button.

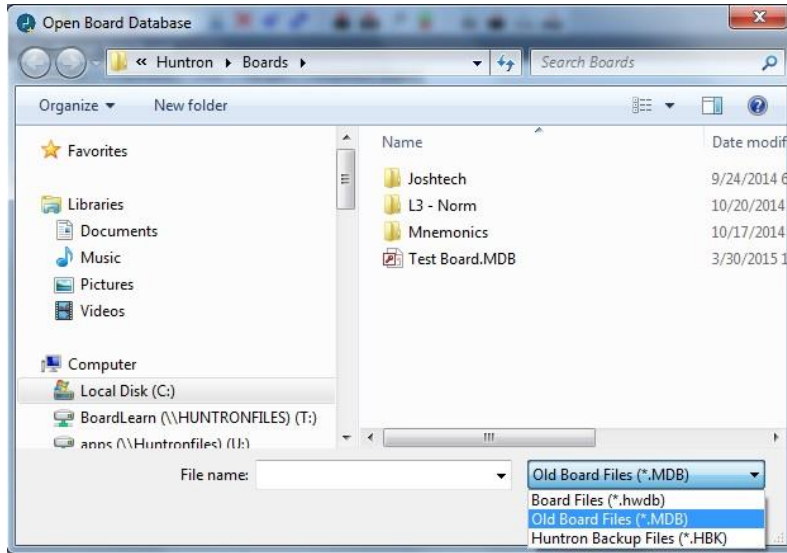

Click the **Convert** button to create the new test for version 4.3. The conversion can take some time based on the original test size.

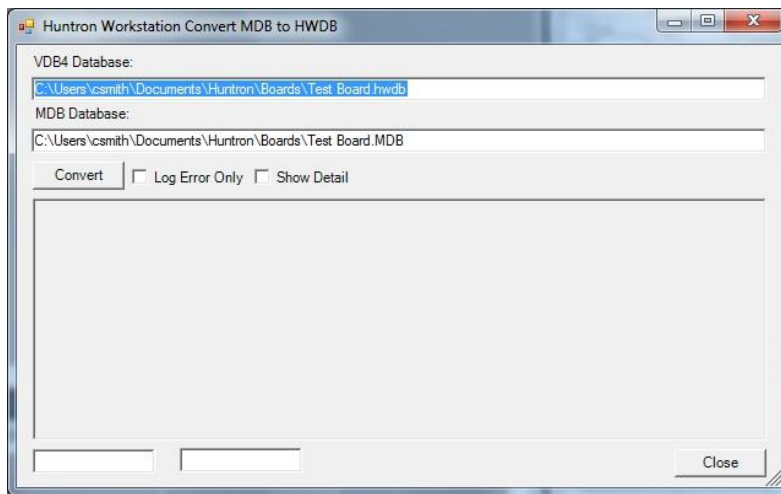

Click the **Close** button when the conversion is complete. The updated test will be opened in the Workstation interface.

Building Procedures for a New Test

- Create Test Database in the Tree Pane
 - o Add Board, Sequence, and Components before teaching or scanning
- Scan Components and Set References (Tracker only or Tracker/Scanner users)

Listed above is a general outline on how you would proceed when preparing to test a board. These guidelines apply to all package types and boards. As with any type of complex test equipment, practice makes perfect so take the time to learn and practice these procedures.

Creating a Board Database

The screenshot shows the 'Add New Board' dialog box. It has a title bar 'Add New Board'. The main area contains two columns of input fields. The left column includes: Name (Power Supply), Revision, System (Controller), Unit, Top Name (Top), a checkbox for 'Show Instructions', 'Load CC File...', and 'Remove CC File...'. The right column includes: Manufacturer (Huntron), Test Routine Number, Unit of Measure (Mils), Data Source (User), Bottom Name (Bottom), Instructions Id, and CC File Id. On the right side of the dialog are buttons for 'OK', 'Cancel', 'Buttons...', and 'Help'. At the bottom, there is a tabbed area with 'Instructions' selected, showing a text area with the word 'Prober'.

To create a new Board, select **New** from the File menu or use the **New** button in the toolbar. Input information into the "Add New Board" dialog as needed. The only field that is required is board **Name**. Other fields such as Revision, System, Unit, Manufacturer, Test Routine Number can be completed with related information if desired. Instructions can be added in the Instruction field now or added later.

Adding a New Sequence

To add a new Sequence, select the **Sequence** tab in the Tree pane. Select **Add New Sequence** from the Edit menu or click the Add New button (+) in the toolbar.

Primary Details:

Sequence Name Field: Enter Sequence name

Compare Priority: Selects the comparison priority of signatures to Reference signatures between **Same** (serial number as Reference), **All** (All References; this is the recommended setting) or **Merge** (Merged min/max signatures)

Slot: This selection is used with Access Probers.

Type: Components or **Nets**. Select **Components** for most tests as Net tests are usually created using CAD data.

Side: This selection is used with Access Probers. **Top** is the default.


Instructions field: Enter any instructions or system information that you wish to pass on to future users. Note: the **ENTER** key in this field will work as a carriage return.

The **Delete Scans** button will erase all scans stored under the Sequence.

Other functions within this window can be read about by clicking the **HELP** button.

Adding a New Component

Component Package Types

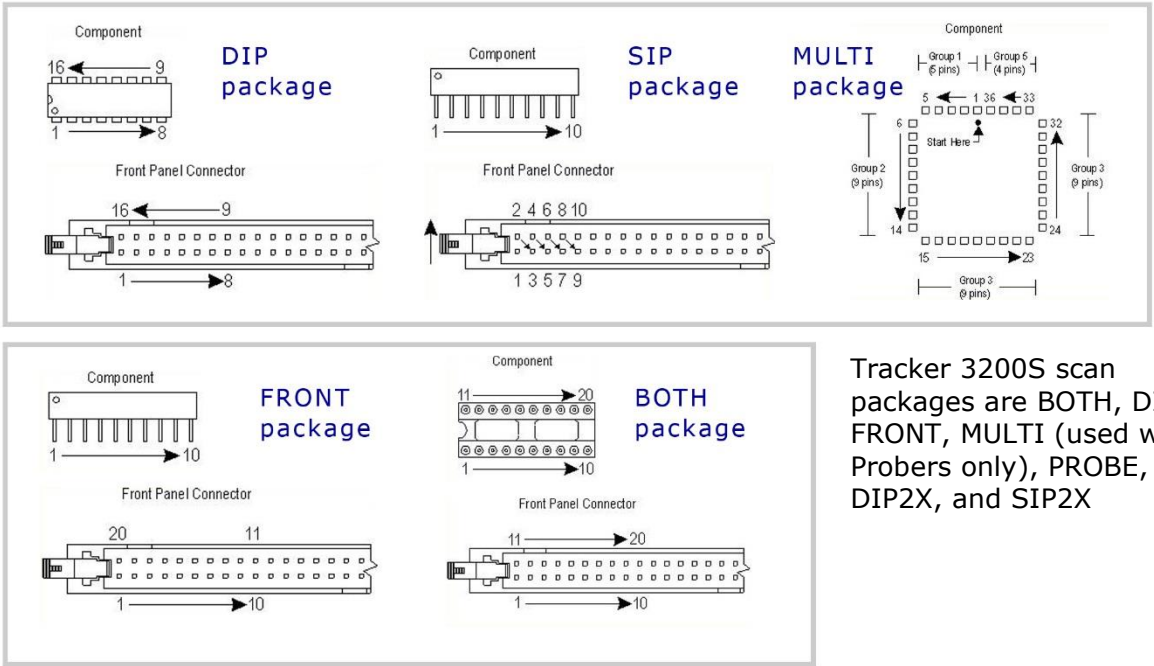

Tracker 3200S scan packages are BOTH, DIP, FRONT, MULTI (used with Probers only), PROBE, SIP, DIP2X, and SIP2X

When adding a new component to your test the package type determines how the front panel Scanner connection pins are counted. The available Scanner packages are **Both, DIP, Front, Probe** (uses manual test probes), **SIP, DIP2X** (combines the A and B channels for 128 pins) and **SIP2X** (combines the A and B channels for 128 pins). There are other packages listed (i.e. Multi, Cable) in the Package drop menu that are used with other Huntron hardware.

To add a new Component, select the **Component** tab in the Tree pane. Select **Add New Component** from the Edit menu or click Add New button (+) in the toolbar.

The screenshot shows the 'Edit Component' dialog box with the following details:

- Component Name:** U1
- Order Number:** 1
- Package:** DIP
- Number Of Pins:** 14
- Type:** 74HC04
- Pin Spacing:** 100
- Connection Type:** Scanner
- Open Check Type:** Rec
- Open Recheck Depth:** 8
- Correction Steps:** 3
- Short Check:** None
- Component ID:** 1
- Sequence ID:** 1

Buttons: OK, Delete Scans, Buttons..., Help.

Details:

Component Name field: Enter the component name (reference designator) in this field.

Package and **Number of Pins** fields: Using the mouse, click on the down arrow to the right of the field to bring up the pull-down menu. Select the package type and number of pins from these menus.

Type field: This information is optional but you can enter the component type in this field.


Connection Type: Select the type of hardware used to interface to the component. Select **Probes** if manual probes will be used or **Scanner** if the front panel Scanner connections will be used.

Instructions field: Enter any instructions or component information that you wish to pass on to future users.

Other functions within this window can be read about by clicking the HELP button. Click the **OK** button to close the Edit window.

Tree/Pin Tab

Once a component is added to the Workstation Tree, switching to the Pin tab will display information for each pin of the selected component.

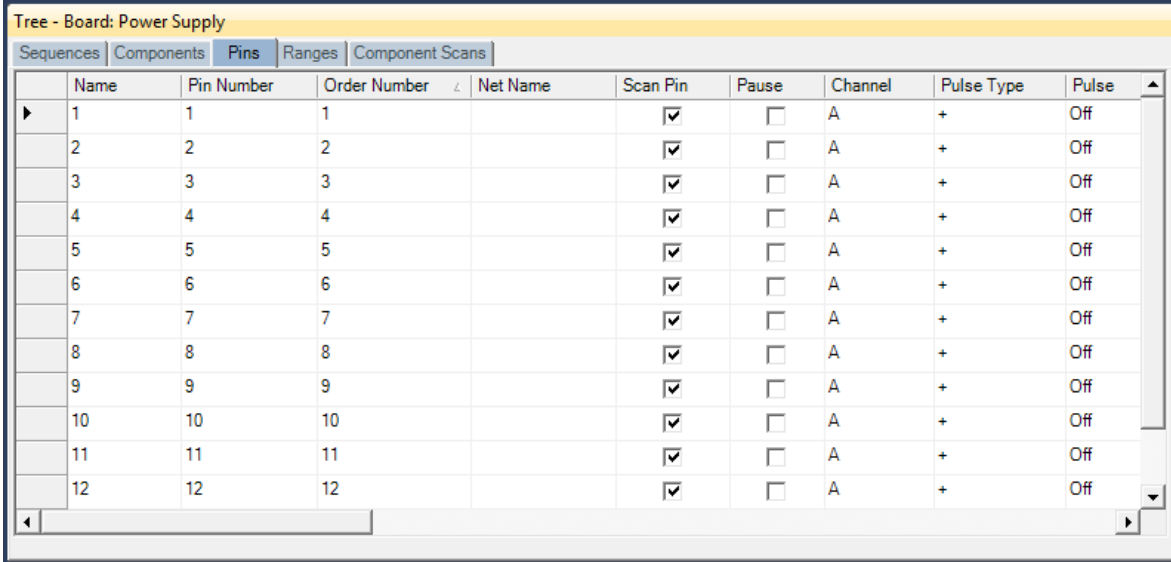


| | Name | Pin Number | Order Number | Net Name | Scan Pin | Pause | Channel | Pulse Type | Pulse |
|---|------|------------|--------------|----------|-------------------------------------|--------------------------|---------|------------|-------|
| ▶ | 1 | 1 | 1 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 2 | 2 | 2 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 3 | 3 | 3 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 4 | 4 | 4 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 5 | 5 | 5 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 6 | 6 | 6 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 7 | 7 | 7 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 8 | 8 | 8 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 9 | 9 | 9 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 10 | 10 | 10 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 11 | 11 | 11 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |
| | 12 | 12 | 12 | | <input checked="" type="checkbox"/> | <input type="checkbox"/> | A | + | Off |

Text in the **Name** field can be modified directly by clicking in the text field and typing the new name. The **Scan Pin** setting enables or disables scanning of the pin. **Pause** will cause the scan to pause when the selected pin is reached. The **Channel** field controls which channel (**A or B**) is used. Controls for the Tracker Pulse Generator can also be controlled at the Pin level. These control include **Pulse Type** (polarity), **Pulse** (on/off), **Pulse Level** (amplitude) and **Duty Cycle** (up to 50% on pulsed signals). Consult the Tracker 3200S User's Manual for how the Pulse Generator is used. Information on the other settings in the Pin tab is available in the **Workstation Help**.

Adding a New Range


When a new component is added to a Sequence the ranges used are set by the defaults set up in the **Tools/Options/Ranges** tab. It is best to set up your desired default ranges before adding Components to your Sequence.

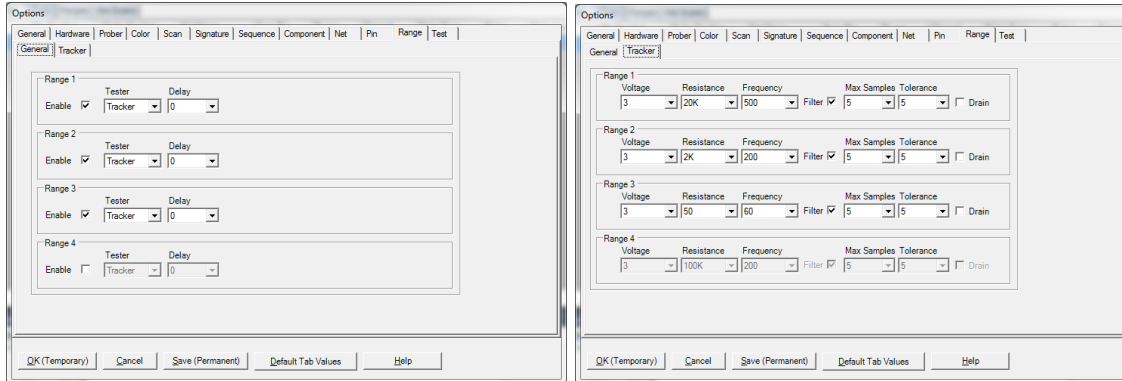


In the Range/General tab, enable the number ranges and set the tester type as Tracker (default). In the Ranges tab, set the Voltage, Resistance and Frequency range parameters. These are the ranges that will be used when adding a new Component. It does not change existing Components. On a new software installation these defaults set three ranges – **3V, 50Kohms at 500Hz; 3V, 1Kohms at 200Hz** and **3V, 50 ohms at 60Hz**. In general use, these three ranges will work well but you may need to add or modify ranges based on component type and value. As a general reference, the table below can be used to assist you in setting ranges.

| Range | Voltage>
200mV | 3V | 6V | 10V -15V | 20V |
|--------------------------|--|---|---------------------|--|---------------------------------------|
| Impedance↓
10Ω - 100Ω | continuity,
shorts, caps,
resistors &
inductors | low
impedance
components | newer MOS
ICs | power supply
& regulators | |
| 1KΩ - 10KΩ | resistive
faults | latest MOS &
surface
mount
ICs | newer MOS
ICs | older MOS ICs | |
| 20KΩ | resistive
faults | resistive
faults | older MOS
ICs | TTL 74XXX &
74LSXXX ICs,
older MOS Ics | TTL 74XXX
ICs, power
transistor |
| 100KΩ | resistive
faults | resistive
faults | resistive
faults | resistive faults | Hi resistance&
Hi power |


The Tracker signatures are shaped based on the Tracker range settings. The basic goal is to achieve signatures that are halfway between open and short. The signatures for the four basic types of components shown below illustrate this primary goal.

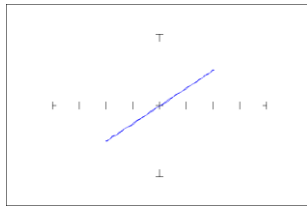


Resistance

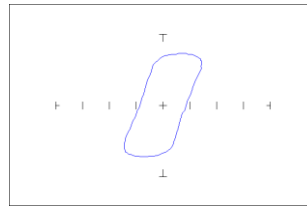

Inductance

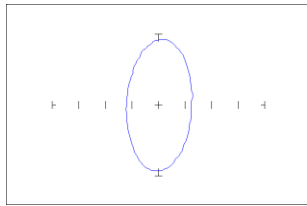

Capacitance

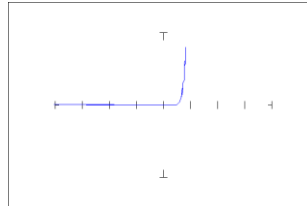

Semi-conductance

Select the Tree/Range tab to display the ranges for the selected component pin. RIGHT click on the row header (far left grey area of the row) to display a quick menu (shown left)

To add a new Range, select the Range tab in the Tree pane. Select **Add New Range** from the Edit menu or click the Add New button (+) in the toolbar. A pop-up dialog will

ask where you want the new range to be added. Select the desired radio button (**All Pins** is generally the desired selection) and click **OK**.

Add New Range Details:

Note: **Voltage/Resistance/Frequency** can be modified directly in the Range grid.

Voltage/Resistance/Frequency fields: Select the desired range settings

Max Samples/Tolerance/Delay: Select the setting to be used when scanning **this range**

Common Pin: Select Scanner common pins to be used when scanning **this range**.


Scanner users wishing to use a particular component pin (i.e. ground pin) for Common should select the Common pin at this time using the **Common Pin 1 field** (the Common Pin 2 field is rarely used).

Note: It is easier to set up the ranges used by selecting **Tools/Options/Range** from the Tools menu in the menu bar and pre-configuring the default ranges.


Scanning with a Tracker 3200S

To scan an entire Sequence, select the Sequence in the Tree/Sequence tab or enable the **Sequence checkbox** in the Scan tab. To scan an individual component, select the component in the Tree/Component tab.

Select the **Scan tab** in the Signatures pane and input a **Serial Number** then click the **Start** button.

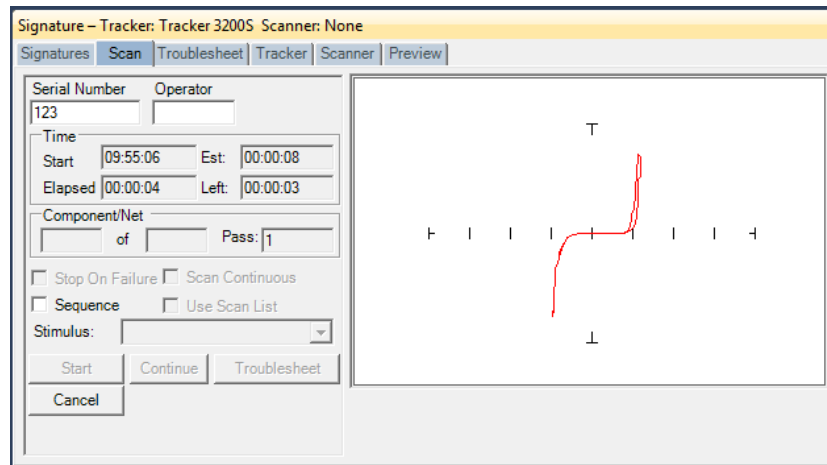


You will be prompted to connect to the component. Tracker with Scanner users should connect to the selected component at this time. Click **OK** to initiate the Scan.

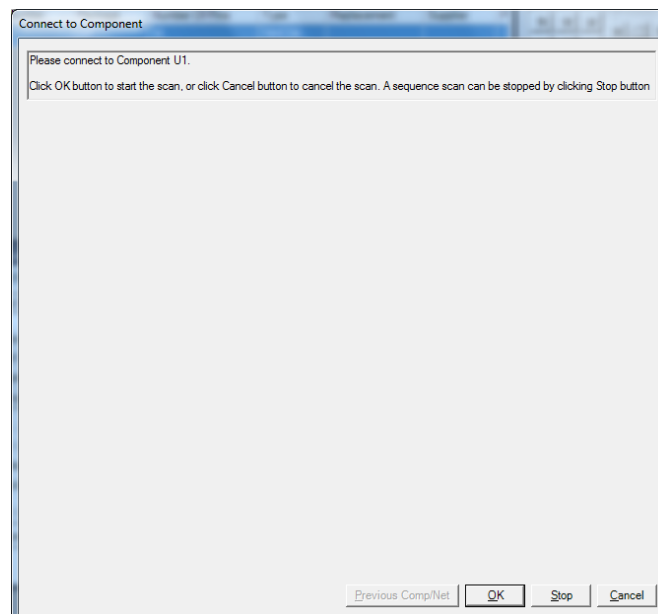

If you are performing Sequence scan you will be prompted to continue to the next component until all of the components in the Sequence have been scanned.

If a Tracker with probes is being used you will be prompted to connect to pin 1 of the selected component (if performing a single component scan) or of the first component in the Sequence (if performing a Sequence scan). Click the **OK** button to scan the first pin. You will then be prompted to move to the next pin for scanning. Click **OK** to scan and continue in this manner until all of the component pins are scanned. At anytime during scanning you can click the **Previous Pin** button to go back and rescan the previous pin.

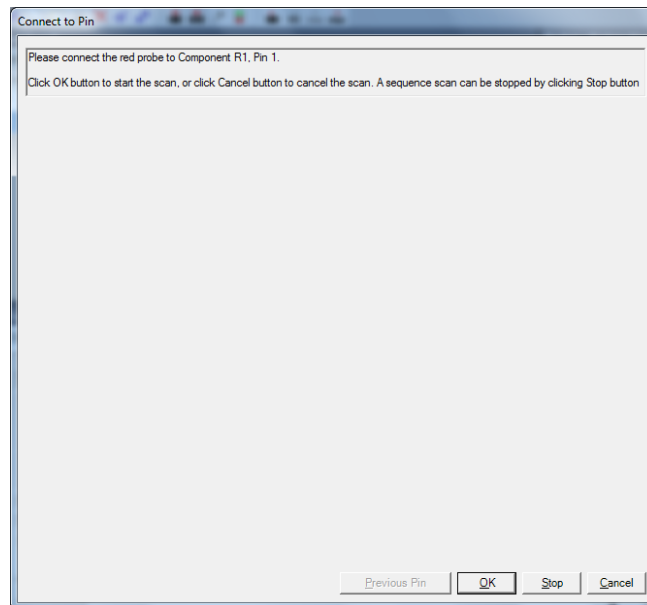


Once all pins are scanned click the **OK** button to continue.

When the Sequence or Component scan is complete the Scan Results window will be displayed. Go to the **Scan Results** section of this tutorial for more information on what to do after scanning.

If the Tracker Scanner connections are being used (i.e. DIP clip and cable) you will be prompted to Connect to the Component before the scan is executed. Connect the Scanner cable to the component to test and click **OK** to start the scan. Once the scan is complete, the Scan results will be displayed.

Scan Results

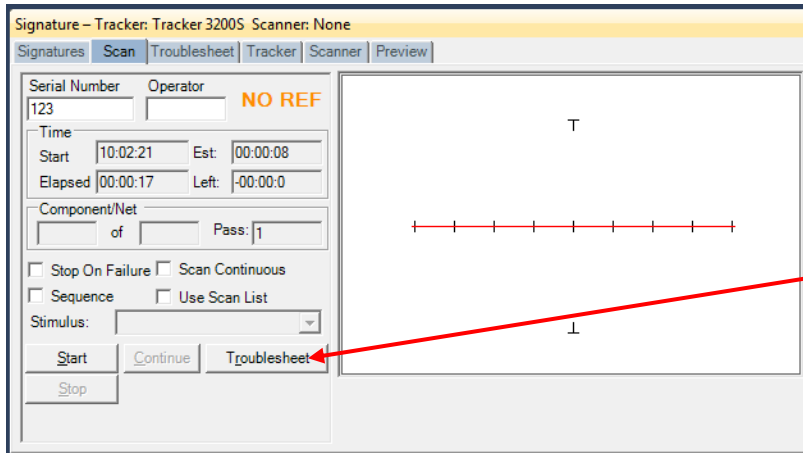


Click the Troubleshoot BUTTON to view latest scan results!

When a scan is complete, the results NO REF, PASSED or FAILED will be displayed (the text of the PASSED or FAILED message can be changed in the

Tools/Options/General settings). The NO REF message will be displayed on the first scan of any test since there are no signatures stored as a comparison Reference.

Clicking the **Troubleshoot** button will display the signature from the last scan in the Troubleshoot tab of the Signature pane.


Note: Selecting the **Troubleshoot** tab will display Troubleshoot information from the previous scan.

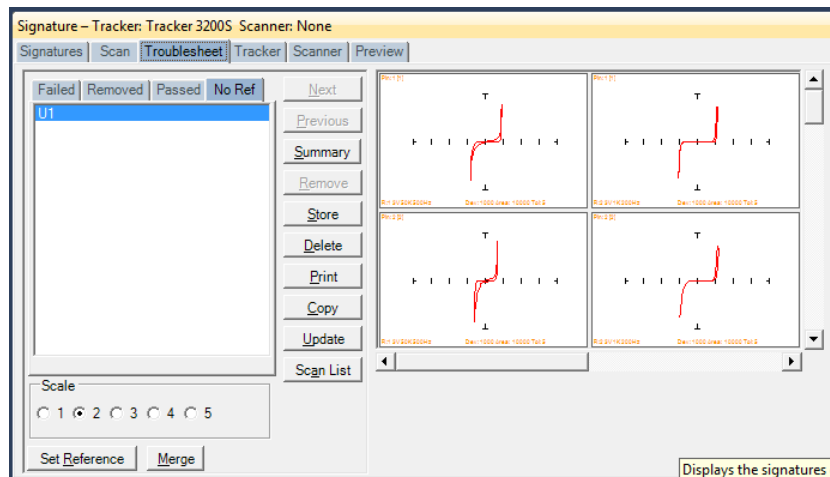

The first NO REF scan will display signatures in red with orange text. Review the signature at this time. If the signatures meet your approval (always use a known good PCB) click the **Set Reference** button to mark these signature as a comparison Reference. The text will change to green when set.


Viewing Signatures – Troubleshoot

Once a test has reference signatures stored, subsequent scans will compare to those references. The test results will be either PASS or FAILED.

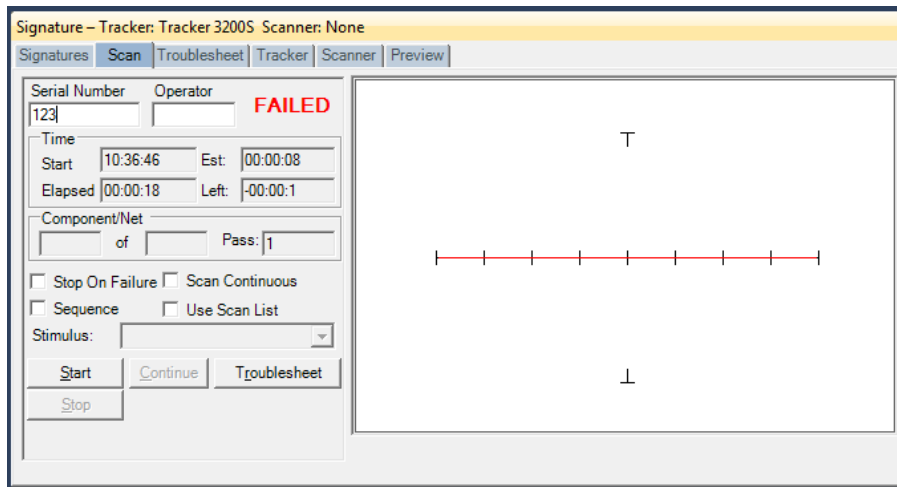

Click the **Troubleshoot** button to see the test results.


When a scan is executed and compared to the Reference signatures, the current scan signatures (in red) will overlay the reference signatures (in green).

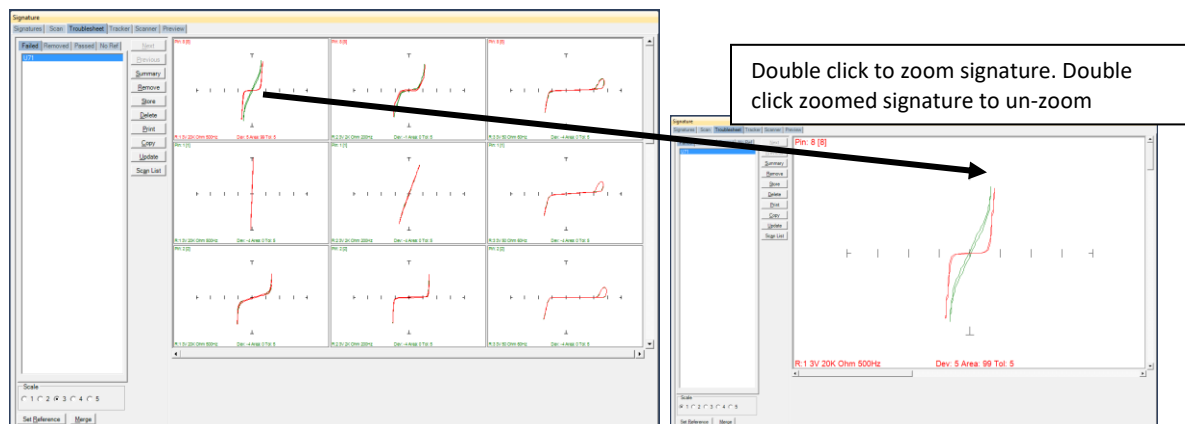


Components that fail comparison will be listed under the Failed tab. Components that pass comparison will be listed in the Passed tab. You can remove components from the list by clicking the **Remove** button where they will be moved to the Removed tab and not included in any Troubleshoot reports. Use the **vertical scroll bar** to scroll through the scanned pins. Use the **horizontal scroll bar** to scroll the pin ranges especially if the viewing is set to **Pin** mode (see Viewing Signatures – Right Click section).

Viewing Signatures Troubleshoot Report

To view and print the Troubleshoot report, press the **Print** button in the Troubleshoot window.

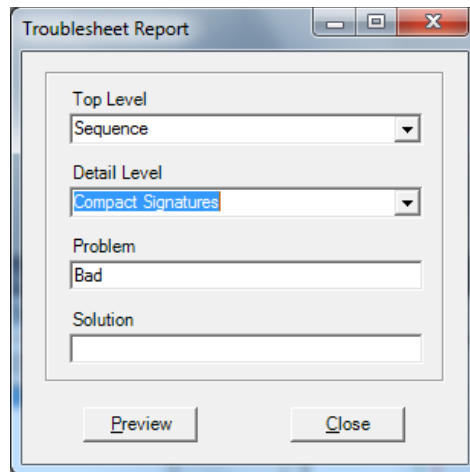


You can select from several options including a Sequence or Component Level report, the level of detail and add problem and solution comments to the report. Click **Preview** to view the report on-screen.

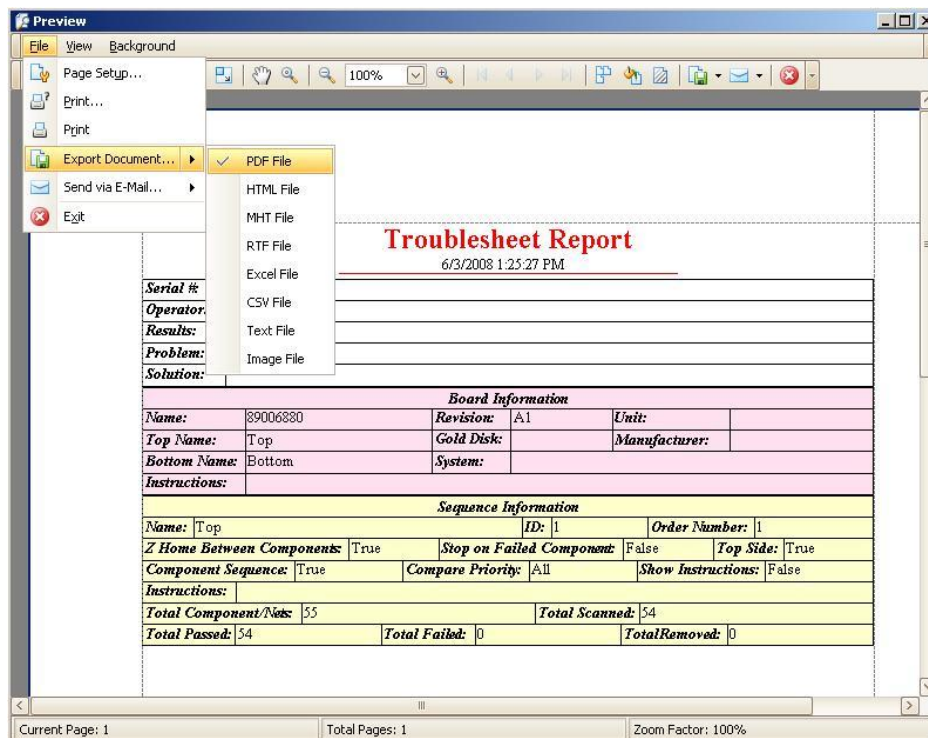


The report can be printed or exported in several different formats including HTML and PDF by selecting **File/Export Document** in the Preview window.

Viewing Signatures in the Signatures Pane

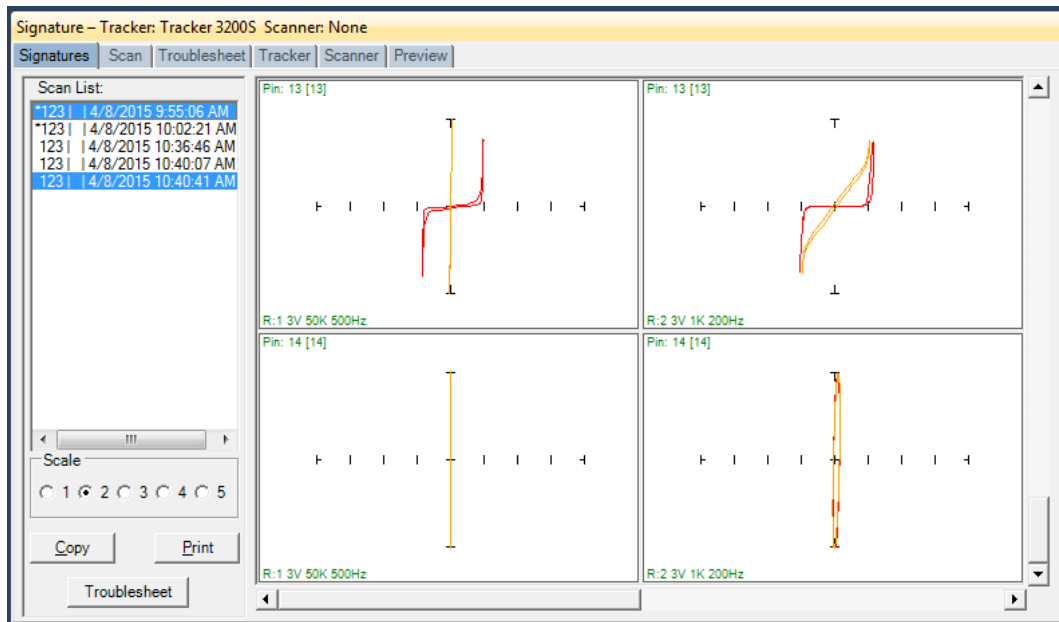

To view scanned signatures of the component selected in the Tree pane/Components tab, select the **Signatures** tab in the Signature Pane. The Scan name, date and time will be displayed on the left side of the window and signatures on the right. The **Scale** buttons will change the number of columns displayed. Scaling the window will increase the number of signatures displayed. The **Copy** button will copy the signatures to the Windows clipboard so they can be pasted into another program (in a metafile format). The **Print** button will print the signatures in one of several different user selected formats. The **Troubleshoot** button will switch to the Troubleshoot tab and display the Troubleshoot of the scan selected in the Scan List. You can use the keyboard **Shift** and **Ctrl** keys to select and stack signatures in the signature boxes (shown above). The signatures will be displayed in contrasting colors and can be very useful if you want to make general comparisons among different scans.

Viewing Signatures – Right Click

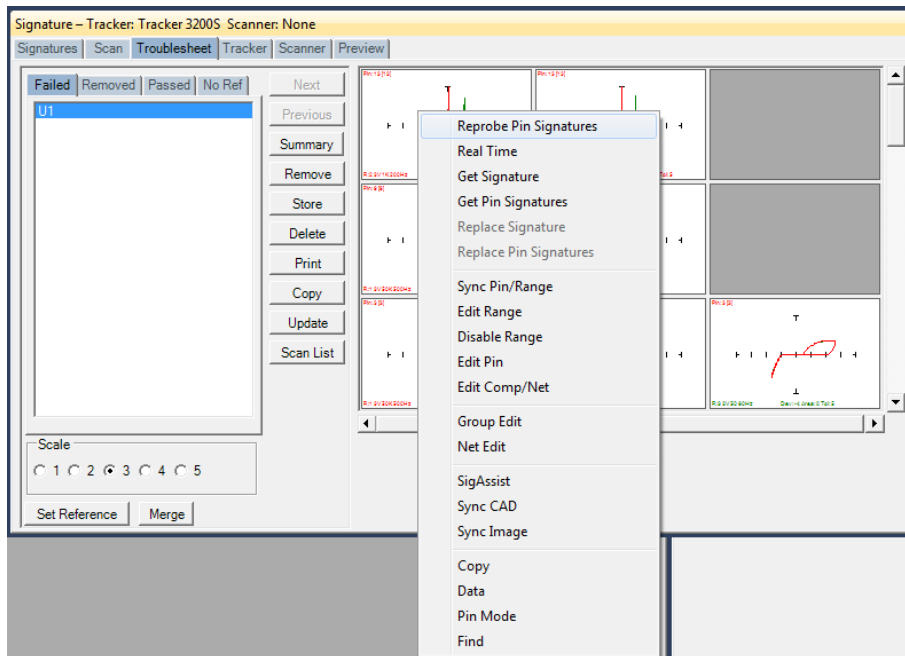

Additional options when viewing signatures can be displayed by right clicking in the signature area.

Reprobe Pin Signatures: Capture signatures for all displayed ranges and prompts to replace signatures immediately – available in Range mode only

Real Time: Display signature in real time

Get Signature: Capture signature for selected pin and range

Get Pin Signatures: Captures signature for all ranges – works only in Range Mode

Replace Signature: Replaces the current signature with the captured signature displayed for the selected pin, range and scan (shown in the Scan List to the left)

Replace Pin Signatures: Replaces the current signatures with the captured signatures displayed for the selected pin, all ranges and scan – works only in Range Mode

Sync Pin/Range: Selects pin and range in the Tree (see default in Tools/Options)

Edit Range: Selects the pin and range in the Tree and opens the Edit Range dialog

Disable Range: Disables the selected range (set in the Tree pane, Ranges tab)


Edit Pin: Selects the Pin the in the Tree and opens the Edit Pin dialog

Edit Comp/Net: Shortcut to the selected Component Edit dialog in the Tree pane

Group Edit: Opens Group Edit dialog for editing of component pin parameters as a group

- Net Edit:** Opens Net Edit dialog for editing of Net pin parameters as a group
- SigAssist:** Displays the SigAssist window showing calculated approximate values of resistance, capacitance, breakdown voltage, etc. based on signature information
- Sync CAD:** Will link the selected signature to the CAD image displayed in the Image/CAD pane. **Sync CAD** will be disabled if there is no linked CAD data.
- Sync Image:** Links current Troubleshoot to the image in the Image pane/Image tab
- Copy:** Places the signature image in the clipboard
- Data:** Displays the signatures numeric data
- Range/Pin Mode:** Displays signatures with Range priority or Pin priority - see default in Tools menu/Options/Signature tab)
- Find:** Searches for a specific component in the Troubleshoot list.

View SigAssist Information

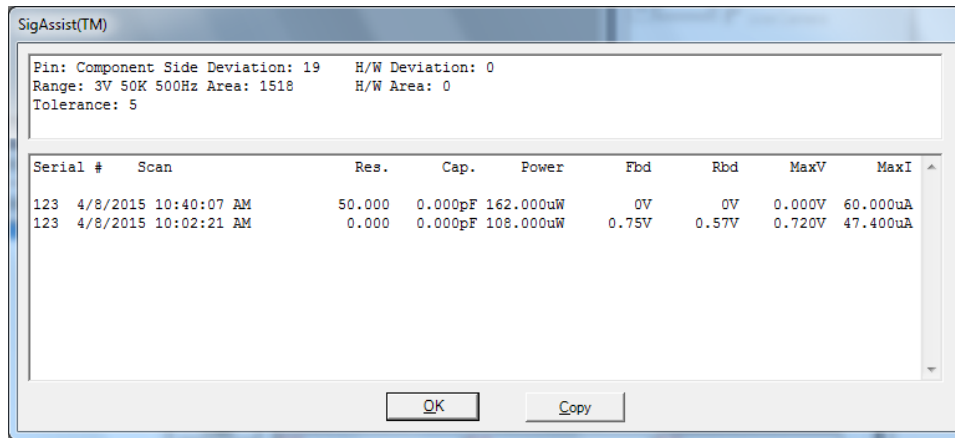

The SigAssist window can be viewed by right-clicking on a displayed signature and selecting SigAssist. It appears as an additional pop-up window. The information presented relates to the individual scans displayed in the signature. The calculated resistance, capacitance, power, forward breakdown voltage (Fbd), reverse breakdown voltage (Rbd), maximum voltage and maximum current are displayed. These values are for troubleshooting purposes only and are not intended to be used as true measurements. The accuracy of the SigAssist values depends greatly on the scanned signature information. SigAssist values may not be calculated for signatures that do not contain enough information for reasonable calculations to take place (i.e. opens, shorts). The Copy button will put a copy of the window into the clipboard for use in other programs.

Component Scans Information

| Tree - Board: Power Supply | | | | | | | | |
|---|----------|---------------------------------------|-------------|--------------------------|-------------------------------------|-------------------------------------|--------------------------|--|
| Sequences Components Pins Ranges Component Scans | | | | | | | | |
| Serial Number | Operator | Scan Date Time | Stimulus Id | Merged | Reference | Passed | Removed | |
| 123 | | Wednesday, April 08, 2015 10:02:21 AM | 0 | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | |
| 123 | | Wednesday, April 08, 2015 9:55:06 AM | 0 | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | |
| 123 | | Wednesday, April 08, 2015 10:36:46 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | |
| 123 | | Wednesday, April 08, 2015 10:40:41 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | |
| ▶ 123 | | Wednesday, April 08, 2015 10:40:07 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | |


Selecting the **Component Scans** tab in the Tree Pane will display all of the scans performed on **the selected component** in a table format. The Scan information displayed includes the serial number, operator, date/time, Merge setting (checked if this scan is included in the Merge set), Reference setting (checked indicates it is set as a comparison Reference), Pass status (will be checked if components passed comparison), Removed status (will be checked if component was removed from Troubleshoot), Area number (highest of scanned pins), Deviation, Min/Max status and other settings (see Help for more information).

Component Scans – Right Clicking (Auxiliary menus)

| Serial Number | Operator | Scan Date Time | Stimulus Id | Merged | Reference | Passed | Removed |
|---------------|----------|----------------------------|-------------|--------------------------|-------------------------------------|-------------------------------------|--------------------------|
| 122 | | April 08, 2015 10:02:21 AM | 0 | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> |
| | | April 08, 2015 9:55:06 AM | 0 | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| | | April 08, 2015 10:36:46 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| | | April 08, 2015 10:40:41 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| | | April 08, 2015 10:40:07 AM | 0 | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |

Right clicking on the Row bar of the Component Scans tab displays an additional menu for performing specific tasks such as enabling/disabling References, deleting a scan for the selected components or all components and loading a Troubleshoot. **Enable Sequence Reference** will mark the scan as a Reference for the entire Sequence. **Disable Sequence Scan** will disable the selected Sequence as a reference. **Delete Scan** will erase the selected scan for the current component only. **Delete Scan All Components/Nets** will erase the selected scan for all components or nets in the Sequence. **Load Troubleshoot** will display the selected scan in the Signatures/Troubleshoot pane.

Component Scans – Right Clicking (Auxiliary menus)

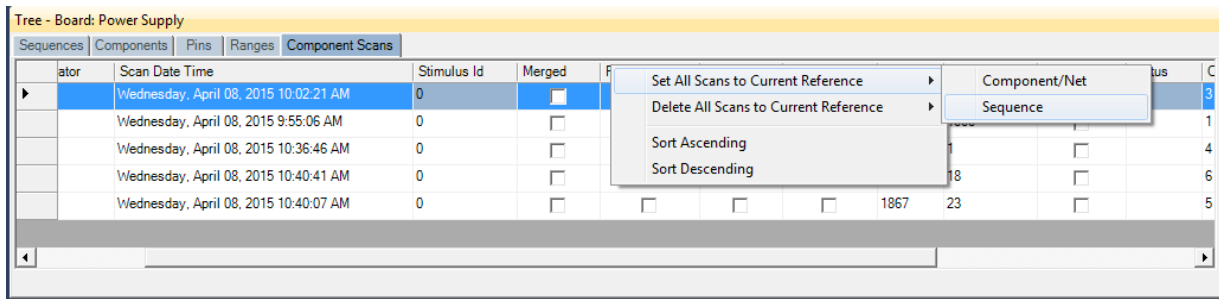

Right clicking on the Column bar of the Component Scans pane displays an additional menu for performing specific tasks such as sorting or globally setting parameters. The menu will vary depending on the column selected. In the image above, the Reference column header was right-clicked.

This method is the easiest way to delete non-reference scans that are listed in the Tree/Component Scans pane. Select a scan that is a non-reference (the Reference check box is unchecked) the right-click the column as shown above. Select **Delete All Scans to Current Reference/Component/Net** or **Sequence** to delete the non-reference scans for the individual Component/Net or for the entire Sequence.


Component Scans – Right Clicking (Auxiliary menus)

The screenshot shows a software window titled "Tree - Board: P/N: S008656 Revision: B4". The "Component Scans" tab is active. A table displays scan data with columns: Serial Number, Operator, Scan Date Time, Stimulus, Merged, Reference, and Passed. A context menu is open over the "Serial Number" column header, showing options: "Set Serial Number Same Date/Time Scans", "Sort Ascending", and "Sort Descending".

| Serial Number | Operator | Scan Date Time | Stimulus | Merged | Reference | Passed |
|--------------------|----------|--|----------|--------------------------|-------------------------------------|-------------------------------------|
| 260-0 | | 13:22 AM | None | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> |
| suspe | | 2:39:20 PM | None | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| suspe | | 2:56:45 PM | None | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| suspect1 | | Wednesday, October 29, 2014 3:34:30 PM | None | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| ▶ suspect 1 pass 2 | | Thursday, October 30, 2014 2:32:29 PM | None | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |


Right clicking on the Column bar of the Scans pane displays an additional menu for performing specific tasks such as sorting or globally deleting items. In the image above, the Serial Number column header was right-clicked.

Sequence/Component/Pin Editing – Right Click menus

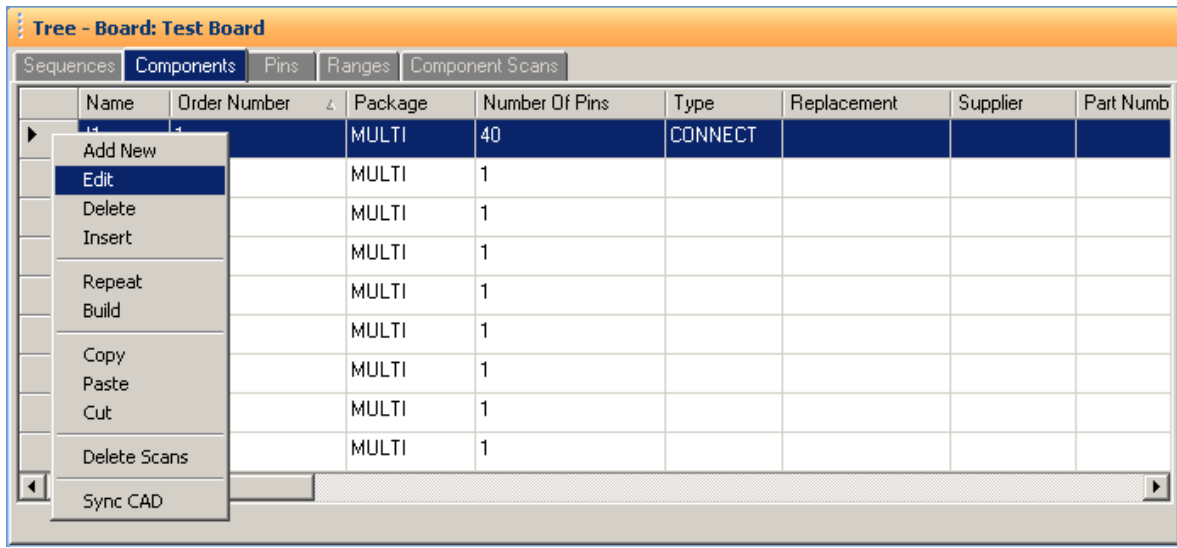


Right clicking on the Row header bar of the Tree pane displays an additional menu for performing specific tasks such as **Add New**, **Insert**, **Delete**, **Repeat**, **Build** (repeat but with name incremented by 1), **Copy**, **Paste** and **Cut**. Right clicking works at all levels of the Tree pane including Sequence, Component (shown above), Pins, Ranges and Scans.

It is also possible to select groups of components by holding the **SHIFT** or **CTRL** keys while selecting components in the Tree. To copy, paste, cut or delete groups of components, use the Copy, Paste, Cut or Delete Toolbar buttons below the main menu.

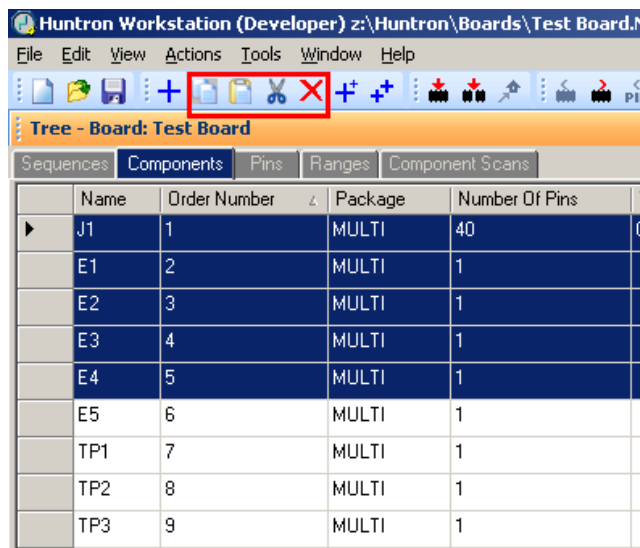


Pin Editing – Right Clicking (Auxiliary menus)

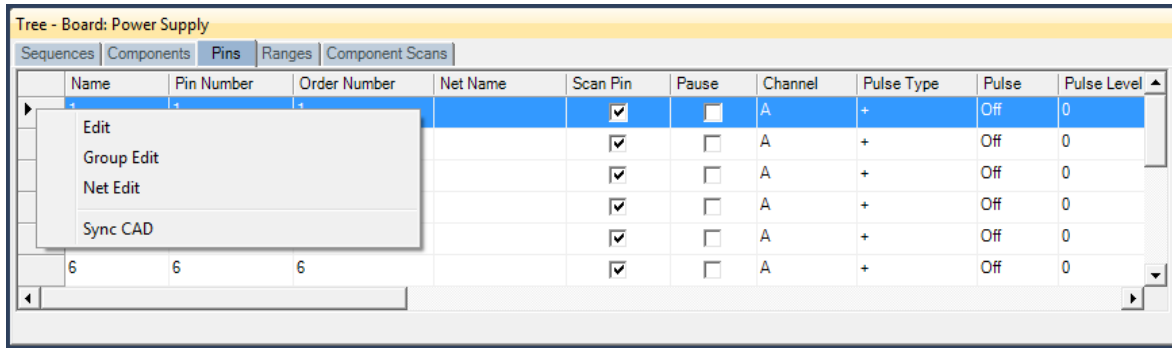

Right clicking on the Row header bar of the Tree/Pins pane allows for editing of the pin information. Select **Edit** to open the Edit window for the selected pin.


Note: Some Pin settings can also be edited directly in the Pins grid by clicking the appropriate field and modifying the setting.

Group Edit and **Net Edit** allow you make changes to the pin of a component and have those modifications also change components that have the same number of pins within the same Sequence.

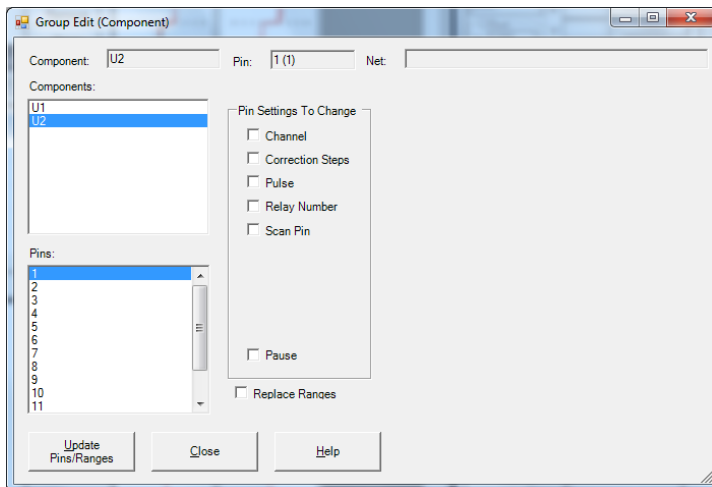

Change the desired settings for the current Pin **first** then select Group Edit from the right-click menu (see above). Components with the same number of pins will be listed. Select the components and pins you want to be changed. Select the Pin Settings check box(s) for the setting(s) you want changed. Check the Ranges box to match the ranges (this will cause signatures to be deleted). Click the **Update Pins/Ranges** button to make the changes.

Pin Editing

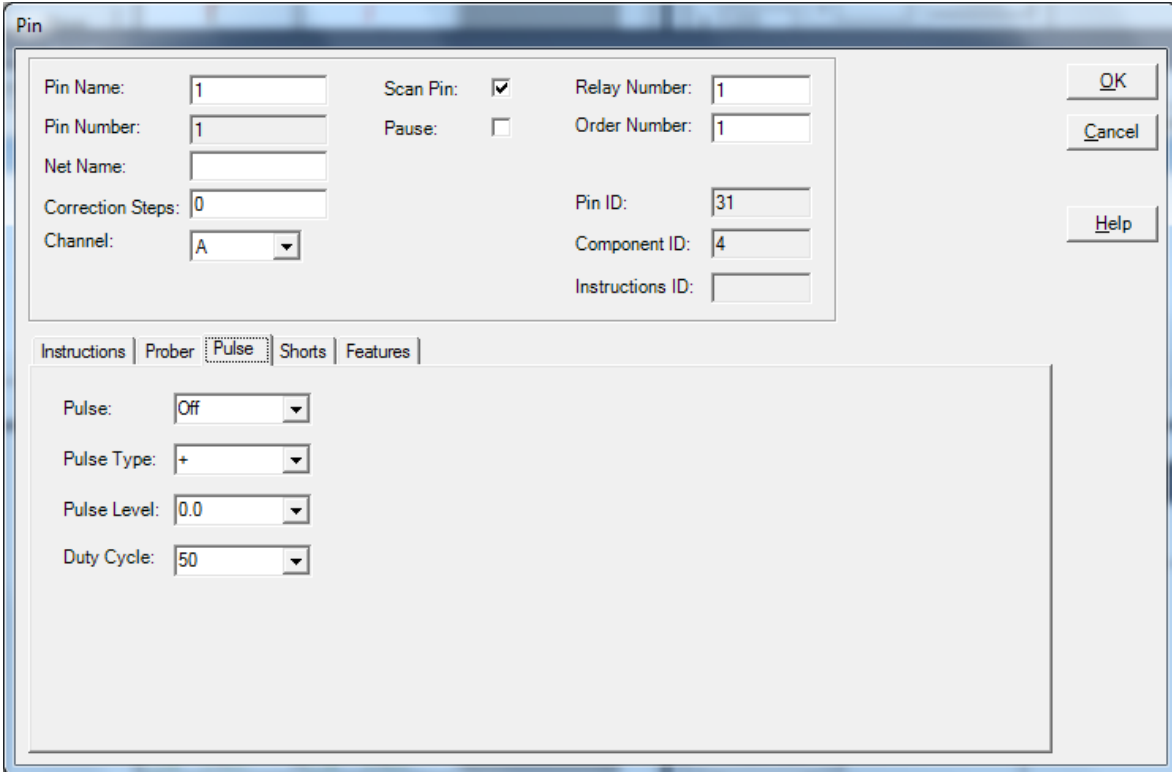

The screenshot shows a software window titled "Pin" with a light blue border. The window contains several input fields and checkboxes. On the right side, there are three buttons: "OK", "Cancel", and "Help". Below the main input area, there are four tabs: "Instructions", "Prober", "Pulse", and "Shorts", with "Pulse" currently selected. The "Pulse" tab contains four dropdown menus for "Pulse", "Pulse Type", "Pulse Level", and "Duty Cycle".

| | | | | | |
|-------------------|---|-----------|-------------------------------------|------------------|----|
| Pin Name: | 1 | Scan Pin: | <input checked="" type="checkbox"/> | Relay Number: | 1 |
| Pin Number: | 1 | Pause: | <input type="checkbox"/> | Order Number: | 1 |
| Net Name: | | | | | |
| Correction Steps: | 0 | | | Pin ID: | 31 |
| Channel: | A | | | Component ID: | 4 |
| | | | | Instructions ID: | |

Instructions | Prober | **Pulse** | Shorts | Features


Pulse: Off
Pulse Type: +
Pulse Level: 0.0
Duty Cycle: 50

Individual pin characteristics can be edited in the Pin Edit window. **Net name**, **Channel**, **Correction steps** (for Access Probers) and **Scan Pin** (enable/disable scanning of the pin) can be controlled. For ProTrack or Tracker 3200S, you can control the Pulse Generator settings used to enable the Pulse Generator during scanning.

Huntron Workstation Buttons Feature


Huntron Workstation has a built-in feature that allows any Windows based program to be started by clicking a button in the Workstation toolbar. It is very easy to use and a “Button” can be attached to any Board, Sequence or Component/Net. In this example, a Button will be created for a Sequence but the process is the same for the Board and Component/Net levels.

To start, the Sequence edit window is opened by right-clicking the row header for the desired sequence. The Edit window will be displayed (see below).

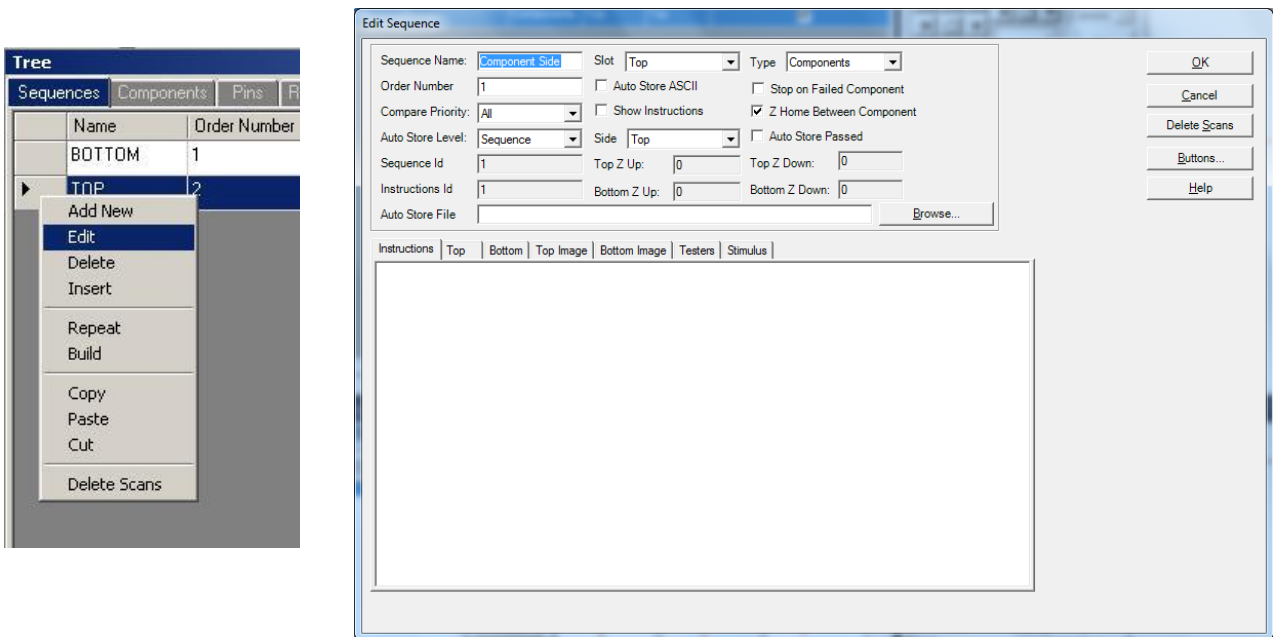

Select the **Buttons...** button located on the right side of the Sequence Edit window to open the Buttons Setup window.

To configure the Button, a Caption (button name displayed in the Tools menu), Command Line (the application to be run) and File Path (the file opened by the executed application) need to be input into the corresponding fields. A File path will not always be required such as instances where a browser is started and pointed to a specific URL. In this example, the button will be configured to start the Microsoft Paint application and open a small PCB image (see image below). If desired, the icon displayed in the main window toolbar can be set by browsing to and setting a path to an .ICO (icon) file in the **Icon File Path** field. Add text that will be displayed when the cursor is placed over the Button in **Tooltip** field. To make the linked file or icon stored as part of the Board database, check the **Store File** and/or **Store Icon** checkboxes.

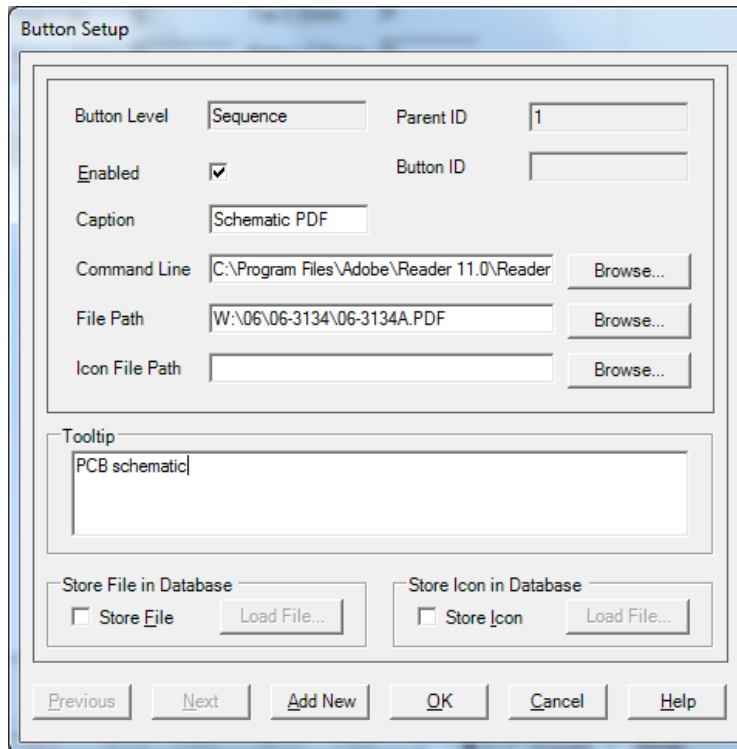

Click **OK** to accept the Button. To create additional Buttons, repeat this process and click the **Add New** button in the Button Setup window.

When Buttons are created, an additional toolbar will appear below the Huntron Workstation menu. This toolbar will change according to the level (board, sequence or component/net) selected.



The icon shown can be replaced by selecting an appropriate icon in the Button Setup window (the default icon is shown). Click the toolbar button to execute the Button.


Technical Support

For questions or assistance in using Huntron Workstation, contact Huntron at 800-426-9265, 425-743-3171 or email info@huntron.com.


There is online assistance for Huntron Workstation at www.huntron.com/support/workstation.htm. This page will contains software updates, a form for reporting software issues and updates to documentation such as this tutorial.

Appendix 1: Huntron Workstation Archive Scans Feature

The new Archive feature built into Huntron Workstation allows you store and remove Sequence scans from the working database to achieve better performance. These archived scans are not deleted but saved away in a different database table and can be restored at any time. It is very simple to use.

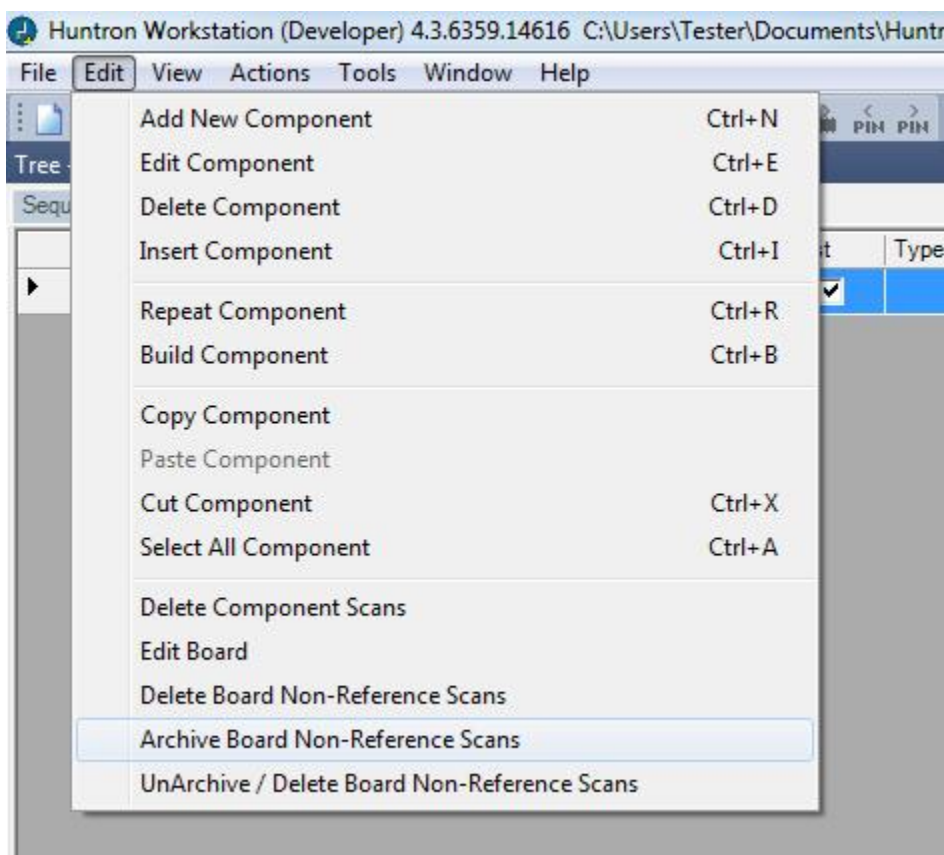

- Select "Archive Board Non-Reference Scans" from the Workstation Edit menu
- At this point the software will search the database for non-reference scans that were part of a Sequence scan and remove them from the active database
- If you look at the Components Scans tab in the Tree pane, you will see that the Reference scans remain
- To unarchive a scan, select "UnArchive / Delete Board Non-Reference Scans"
- The Sequence Scan Archive window will be displayed

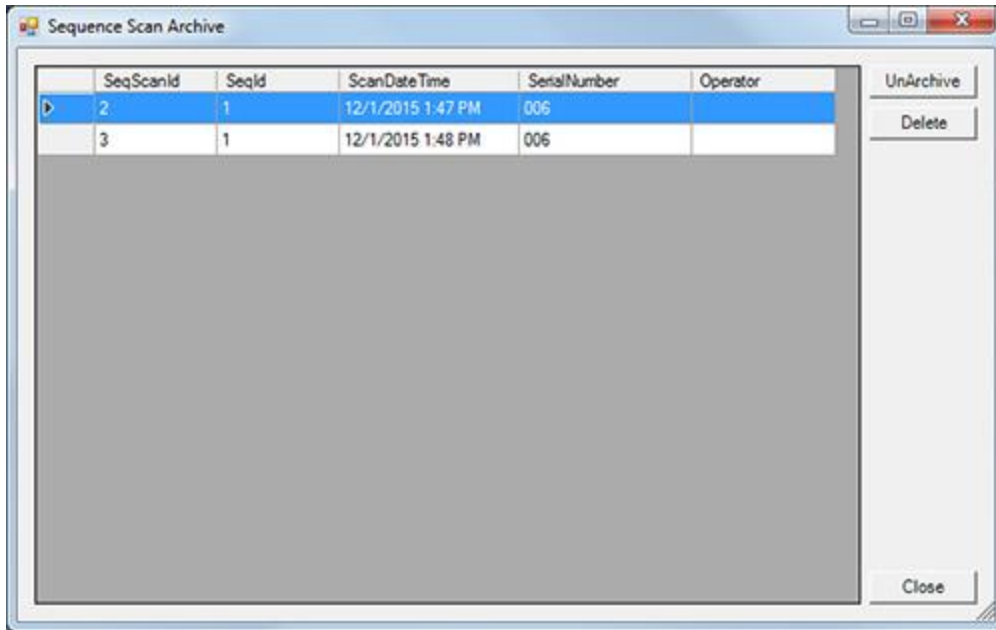


- You will see the Archive Scans listed where you can select the scan you want to restore to your test Sequence. Use the CTRL or Shift keys to select multiple scans if needed
- Click the UnArchive button and the selected scans will be restored to the Sequence
- Use the Delete button to permanently delete scans that are no longer needed.
- Close the Sequence Scan Archive window and look at your Component Scans tab and you will see that your scans have been restored.

Keeping your test database small is the best way to get the most out Huntron Workstation performance.

Appendix 2: Manually Placing Component Tags in the Image Pane/Image tab

Tracker users will appreciate this feature which allows you to manually place tags with the Component name in the board overview image in the Image pane.


You will first need to get a high quality image of your PCB then select the Sequence where you want to use the image. Select **Edit Sequence (Ctrl+E)** from the Edit menu. Select the **Top Image** tab or **Bottom Image** tab depending on the **Side** setting used above (red arrow). Click the **Load...** button and browse to select and **Open** your image.

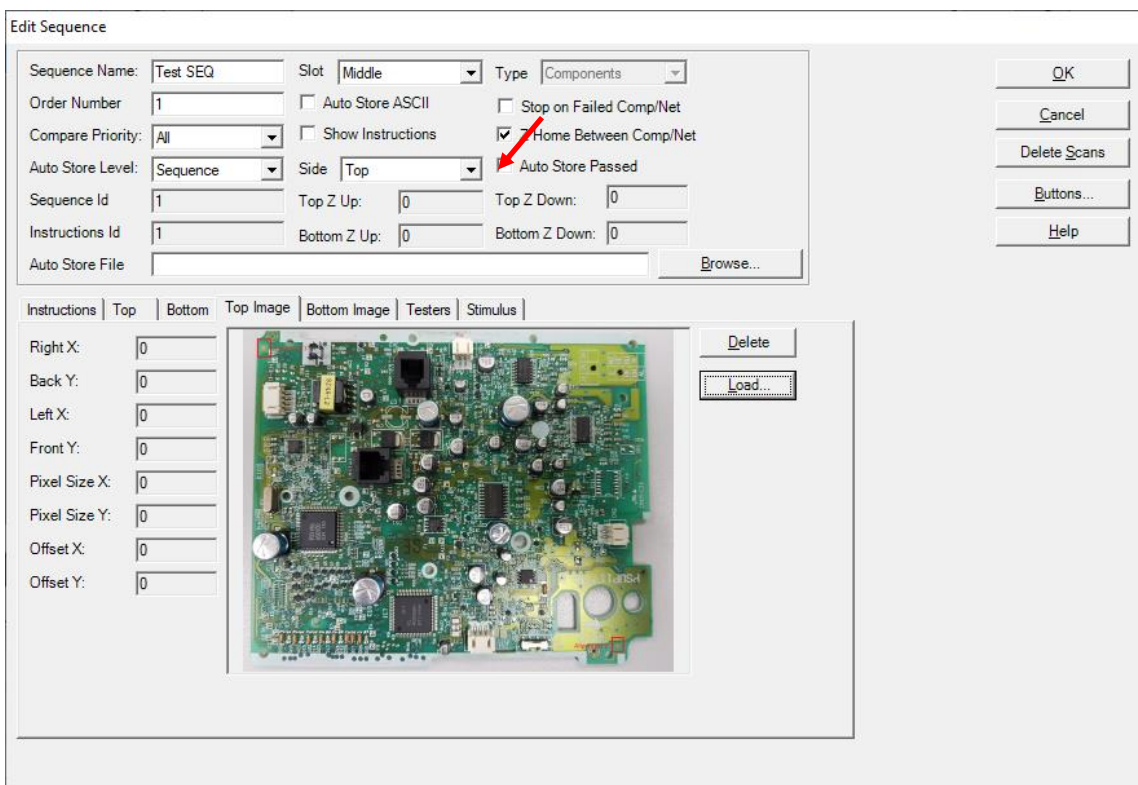

The image should now be displayed in the Top (or Bottom) Image tab. Click **OK** to close the Edit Sequence window.

The image you loaded should now be showing the Image pane/Image tab. If you do not see the Image pane go to the Window menu and select **Image Pane**. You may need to adjust your Workstation layout by click-dragging the panes by the title bar to get the arrangement that suits your needs.

To place a Component name tag in the image, select the Component in the Tree pane/Component tab then **right-click** at the component's location in the image. It is best to click slightly left of center as the text will be left justified. Select **Set Component Position** from the popup menu to place the tag. You should see a grey name tag appear.

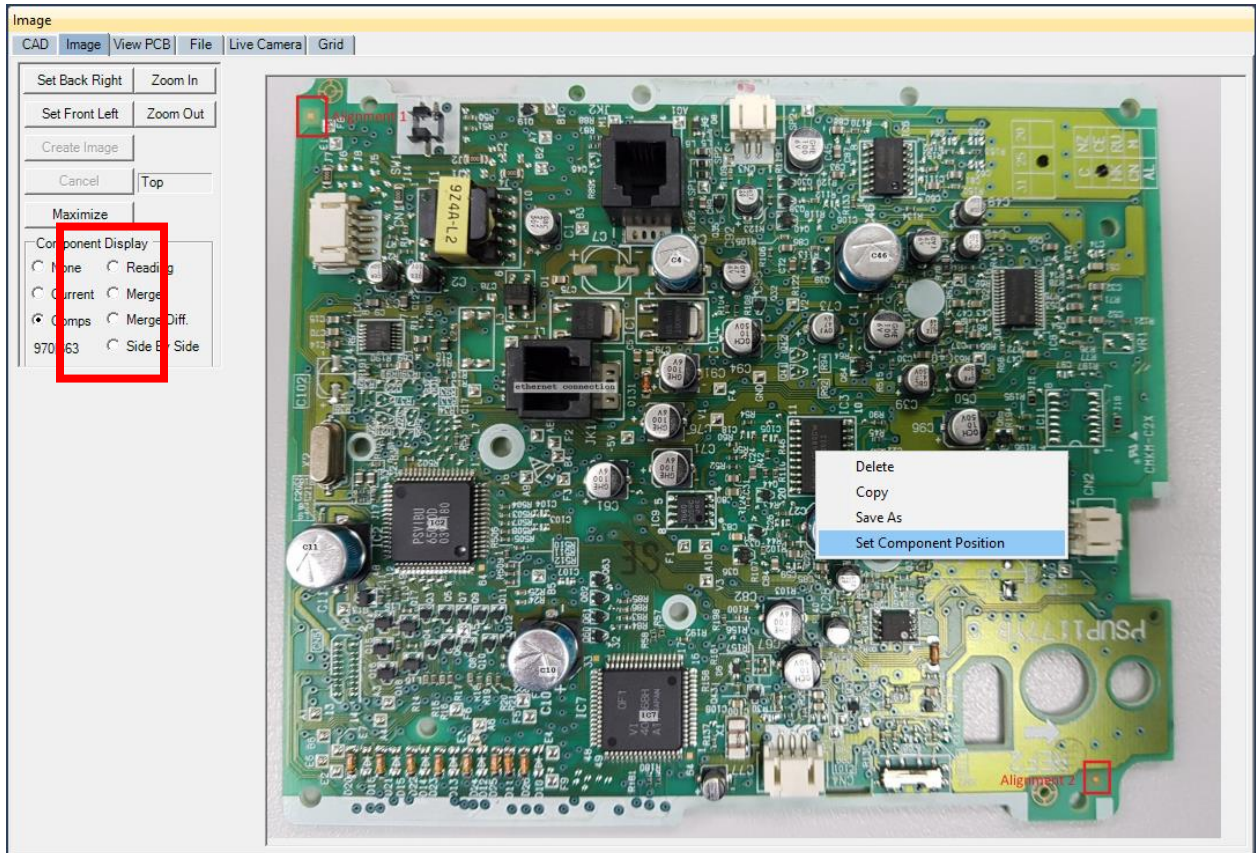

It is recommended you add all of the tags before running any scans. The radio buttons on the left side (red box) control what is displayed in the image. **None** disables the tags, **Current** displays the tag of Components in the current Troubleshoot (green tags for Passed and red tags for Failed) and **Comps** displays all tags in grey.

You can have the tags appear during scanning by selecting the **Tools menu/Options/Scan tab** and enabling **Show Components on Image**. As you run your test, a green (Passed) or red (Failed) tag will appear on the component in the image to indicate its test status. This works the same with Prober systems as well.

